

METHODOLOGY TO USE FLAT-BED IMAGE SCANNER FOR FORMATION ANALYSIS OF PAPER

T. Enomae and S. Kuga

Department of Biomaterial Sciences
Graduate School of Agricultural and Life Sciences
The University of Tokyo
Yayoi 1-1-1, Bunkyo-ku, Tokyo, 113-8657, Japan

ABSTRACT

Versatility of a desk-top flat-bed image scanner with a transparency unit as an image input device for formation analyses was exhibited and discussed. If the scanner output under satisfied prerequisite conditions is calibrated based on a standard film or by comparison to Elrepho type reflectometer, the scanner was found to provide reasonably scaled gray levels. However, there remained some distortion in the output characteristics even after the calibration. So, unlike Elrepho type, optical density squared was almost proportional to the basis weight of paper. Formation of handsheets was quantitatively analyzed with the light transmission images obtained by the scanner. The formation index, the standard deviation of optical density squared correlated better with the subjective ranking than that of optical density or of gray level. Optical density squared divided by the basis weight showed the highest Kendall's coefficient of correlation. Anyway, the standard deviation of gray level was far from propriety as a formation index.

INTRODUCTION

A lot of work on sheet formation analysis of paper have been performed for over sixty years. Through the period of time, image input devices or scanning devices based on a transmission of light had a wide variety. The representative systems so far were the rotating disc of paper with a light spot¹⁾, the Alinco tester using a cathode ray tube whose beam sweeps over an area of up to $44 \times 44 \text{ mm}^2$ by raster^{2, 3)}, the rotating transparent cylinder with a light spot⁴⁾ and video camera systems⁵⁾.

A desk-top flat-bed image scanner is an useful device to obtain image data to a computer. Nowadays, it is prevalently available to many computer users at low costs. In the department of Biomaterial Sciences of the University of Tokyo, analysis of paper sheet formation is one of the major subjects of the juniors' experimental course. The image scanner combined

with a transparency unit has been used since 1995 as an input device of light transmission images in place of a CCD video camera for a formation analysis. Shinozaki⁶⁾ built up an image analysis system mainly for sheet formation, where an image scanner is used as one of input devices. However, he did not discuss how to configure the scanner for reliable images. The purpose of this study is to examine output characteristics of a scanner and to analyze the output images from a viewpoint of formation. The fundamental methodology will be useful for many other possible applications of a scanner for examining paper structure and properties.

MATERIALS

Apparatus

Flat-bed image scanner GT-8500WIN and transparency unit GTA4FLU (Epson Inc., Japan) were used in combination. The working mechanism of the scanner is as follows: RGB xenon fluorescent lights irradiates a sample with three colors of rays. Transmitted (or reflected) light was collected by a lens and detected by an in-line CCD sensor. The sensor is assembled with the fluorescent lights, so they move together in working. The direction of the CCD sensor alignment is called the main scan direction; and that of its movement the sub-scan direction. On the other hand, common CCD video camera systems use a halogen lamp, but uniform illumination is not warranted because a relatively wide area is acquired at one time and external room light may interfere with the destined illumination. A system of a pinpoint beam in combination with a scanning sample stage eliminates this defect, but specific light scattering coefficient depends on basis weight for parallel incidence⁷⁾. This may create different images from those experienced commonly over diffuse light. Furthermore, it takes long time to scan the whole area in two dimensions and the accuracy of positioning is lower. To interface the image scanner to image analysis software, image input driver (software) Epson Scan 32, 2.00J, 1994 was used. The optical resolution was 256 gray levels.

Image analyzer DA-5000S (Oji Scientific Instruments, Japan) and the original software the authors developed using Visual Basic 5.0 (Microsoft Japan) were used to calculate optical density of every pixel in the images for the formation analysis.

Brightness R_{∞} was measured on Elrepho type reflectometer, TD-1800, Tokyo Denshoku, co. Ltd., Tokyo, Japan with D65 diffuse illuminant and normal observer. Opacity R_0 was measured with the same configuration on the same reflectometer with a black cavity backing.

Samples

To ensure the accuracy of the image scanner output, a standard film designed for optical instruments was used. The film was a piece of Density Step Tablet, Fuji Photo Film Co., Ltd., manufactured to measure diffuse visual density. This tablet is a film consisting of portions at several different densities calibrated preliminarily according to Japan Industrial Standard (JIS K 7605).

To compare output characteristics between the scanner and the Elrepho reflectometer, a plastic film 199 μm thick of 178 g/m^2 in basis weight, and tracing paper 41.0 μm thick of 39.3 g/m^2 in basis weight were used. The plastic film was colored blue, but transparent. The tracing paper was of low light scattering for paper, but translucent. Some sheets of them were stacked and loaded slightly by a weight or a scanner cover in measurement.

For an application to formation analysis, handsheets made of softwood or hardwood kraft pulp, loaded with 40 % calcium carbonate to dry pulp, were prepared. Retention time before drainage was 10 (standard-based) or 120 s. Cationic polymer, polyamideamine-epichlorohydrin resin (WS-570, Japan PMC Co., Japan) was added to a half of the samples at 0.4 % to dry pulp. Thus, four kinds (2×2 conditions) of handsheets each were prepared from softwood and hardwood pulps.

METHODS

Configuration of scanner

It was found that there are some requirements of the scanner configuration. They are;

- (1) to cover the rest of the sample area on the document glass stage with an opaque sheet to prevent extra reflected light on the sample surface from coming into the detector,
- (2) to make external lighting uniform in the direction of sub-scan because no calibration is made in this direction to compensate for its non-uniformity, and
- (3) to set input parameters at proper values so that the whole range of optical density for the sample including full transmission out of the sample will fall within the whole input range.

Proper input parameters

In the scanner driver, users can set some input parameters to their purposes. For a formation analysis, one need to set values of γ , highlight and shadow at 1(100 % for this driver) , 255 or higher in some cases and 0, respectively. γ -value is a characteristic curve to determine gain of output to input levels.

This must be linear, namely, 1 for a quantitative analysis. The values of highlight and shadow are a threshold value above which all the levels in input are set at 255 in output, or below which all the levels are set at 0, respectively. So, care must be taken in setting so that the third requirement in the last section is fulfilled. Then, the in-between values are divided into 256 levels at equal intervals.

With the three prerequisites satisfied, the samples were scanned at a resolution of 120 dpi, namely, at ca 0.2 mm intervals. The scanned area was 100 mm \times 100 mm each, but the calculated area was 60 mm \times 60 mm (283 pixel \times 283 pixel) each. The standard film of Density Step Tablet was scanned at the same resolution and the calculated area was 12.7 mm \times 6.4 mm (60 pixel \times 30 pixel). For the plastic film and the tracing paper, almost the same area was measured.

Calculation of optical properties

Optical specification of a sheet, film or any material is likely to be achieved favorably by determining brightness and specific light scattering coefficient. The Kubelka-Munk equation⁸⁾ describes the relation between those parameters. According to it, optical density OD (refereed also to absorbance) is expressed by the equation:

$$OD = -\log\left(\frac{b}{a \sinh bsW + b \cosh bsW}\right), \quad \dots\dots (1)$$

where s is the scattering coefficient, W is the basis weight, and \sinh and \cosh are hyperbolic functions. Likewise, OD of scanner output, that is, gray levels was defined as follows:

$$OD = \log\left(\frac{V_0}{V}\right), \quad \dots\dots (2)$$

where V and V_0 are the gray level of the considered pixel and the gray level in full transmission with no material, respectively. s can be calculated from R_∞ , a and b as follows:

$$s = \frac{1}{bW} \text{Ar ctgh} \frac{1 - aR_0}{bR_0}, \quad \dots\dots (3)$$

$$a = \frac{1}{2} \left(\frac{1}{R_\infty} + R_\infty \right) \text{ and } b = \frac{1}{2} \left(\frac{1}{R_\infty} - R_\infty \right), \quad \dots\dots (4)$$

where R_0 is the reflectance of single sheet with a black cavity backing, R_∞ is the reflectance factor of infinite pile of paper and Ar ctgh is the inverse function of a hyperbolic function, ctgh . But, actually the calculation was made following the modified equation introduced by Hamada⁹⁾.

Radiation of such as β -ray or soft X-ray used commonly for formation analyses tends to attenuate in relation to the local basis weight of paper or distance of the medium through which it is transmitted. Lambert's law below describes the relationship.

$$\log\left(\frac{I_0}{I}\right) = \alpha d, \quad \dots\dots (5)$$

where I , I_0 , α and d are the intensity of the transmitted radiation, the intensity of the incidental radiation, the linear absorption coefficient and the distance of the medium, respectively. The Kubelka-Munk equation reduces to this law if s equals to zero in the derivative form.

Subjective ranking

Subjective ranking was made by 6 panelists with the 8 handsheets in terms of the degree of inhomogeneity in look-through over diffuse white light. The judgement was made by comparing every pair of the sheets. The better one was given 1 point and the total points per sample were calculated. The figure of ranking represents the average point given to the individual sheets. The correlation coefficient of each formation index with the subjective ranking was determined according to Kendall's method. This method is as follow: the same order of each pair with the subjective ranking gives 1 point and the reversed order gives -1 point; the correlation coefficient is expressed in terms of the total points divided by the number of every pair, that is, 28 in this case. This correlation method is advantageous in that it correlates to the ranking order, not to the absolute ranking point that is not reasonably scaled.

RESULTS AND DISCUSSION

Scanner output characteristics

The standard film was scanned by the scanner and optical density OD was calculated. **Figure 1** shows a good agreement of OD measured between by the scanner and by the Elrepho reflectometer up to ca 1. This range roughly means that there is a good linear relationship in gray levels ranging from 25 to 250, for example. The values are also consistent with the pre-calibrated ones noted on the standard film. However, the output characteristics changes over time. After one year, the same standard film was scanned and OD was calculated again. The gradient representing the relationship became much lower, maintaining a good linear relationship (broken line). This may be because the light source has deteriorated. To avoid this possible deterioration, determination of absolute OD values needs calibration as based on a standard film. Scanner of other manufacturers were also confirmed to show a linear relationship.

Figure 2 compares OD measured by the Elrepho reflectometer for the two types of materials; the plastic film and the tracing paper. The OD values of the plastic film (denoted by filled squares) was exactly proportional to the number of sheets. This relationship can be explained by Lambert's law, equation (5), if the number of sheets is assumed to be the

thickness of the material. Lambert's law applies limitedly to the case that the scattering coefficient is negligible. Accordingly, the coefficient was very low (filled triangles). For the tracing paper, OD was not proportional to the number of sheets (open squares). This behavior is typical to paper having many fiber-air interfaces that tend to scatter light (open triangles), as taught by the Kubelka-Munk equation.

OD by the scanner was supposed to provide the same relationship if the agreement found in Figure 1 is taken into

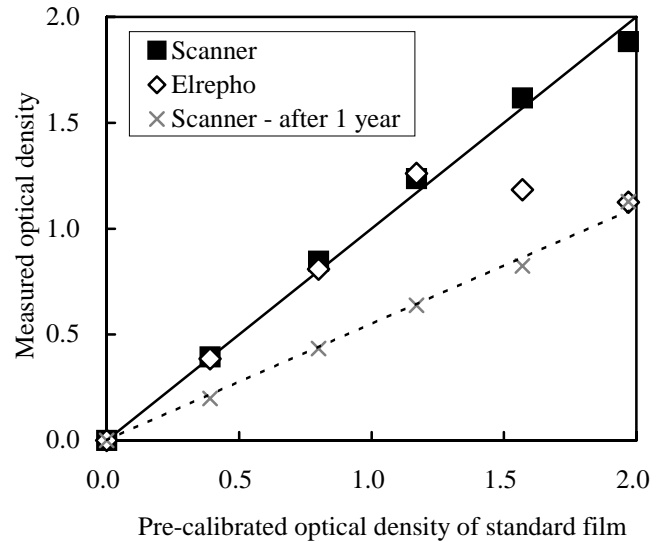


Fig.1 Comparison in optical density of the standard film measured between by scanner and by Elrepho-type reflectometer

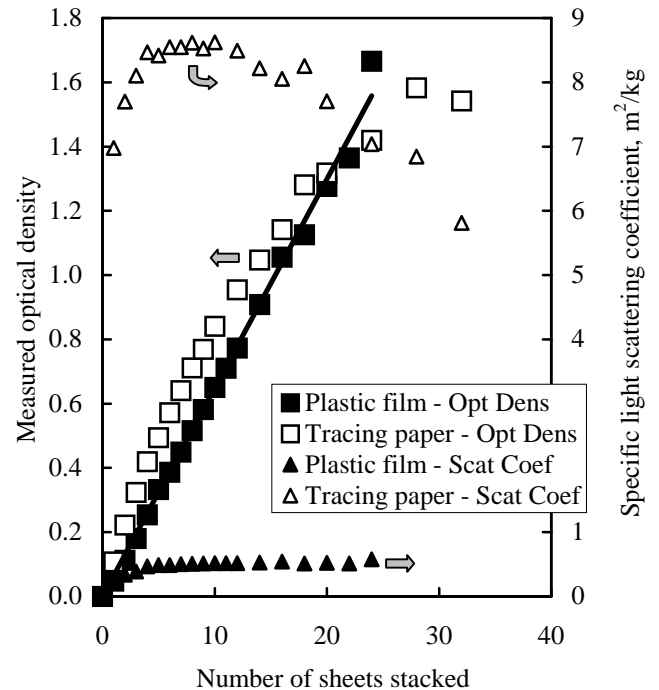


Fig.2 Comparison in optical density measured by Elrepho-type reflectometer between plastic film and tracing paper stacks.

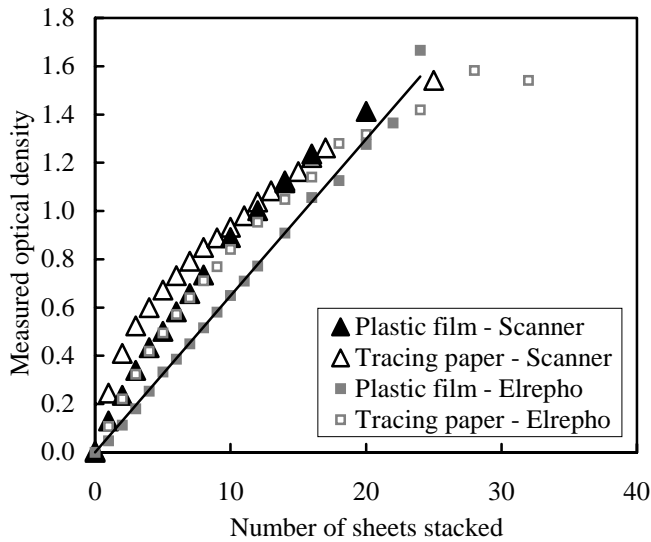


Fig.3 Distortion of scanner output. For the same material stacks, scanner optical density curves upward.

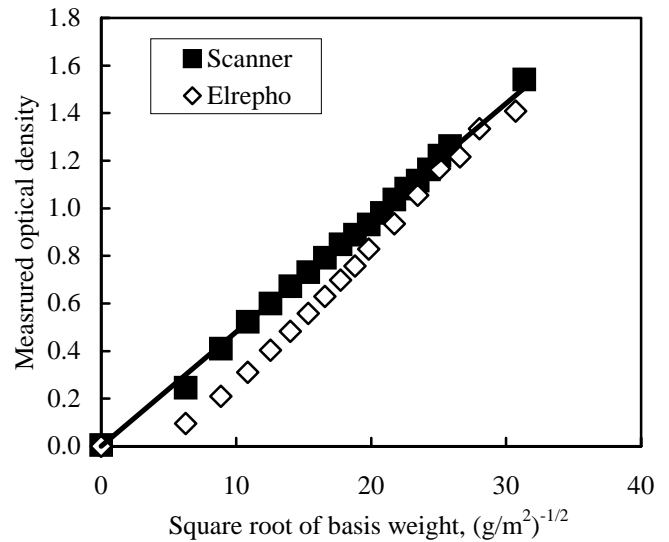


Fig.4 Comparison in optical density of tracing paper stack.

The scanner output is proportional to a square root of the total basis weight.

account. **Figure 3**, however, shows distortion in scanner output. The *OD* is already corrected by the calibration based on the standard film. The gray square plots for the Elrepho output are exactly the same data with in the previous figure. The filled triangle plots for the scanner output curves upward in the middle range. The reason for this is unknown for the present.

Figure 4 shows *OD* as a function of a root of the total

basis weight of the tracing paper stacks, which was easily calculated from the basis weight per single sheet times the number of sheets. The relationship for the scanner is almost proportional to the basis weight, while that for the Elrepho have a linear portion but does not pass through the origin. The proportional relationship for the scanner may be coincidental or may be designed so.

Table 3 Properties and formation analysis results of the handsheets. *r* is Kendall's coefficient of correlation with subjective ranking

Key	HN10	HN120	HP10	HP120	SN10	SN120	SP10	SP120	<i>r</i>
Furnish	Hardwood				Softwood				
Cationic polymer	None	None	Added	Added	None	None	Added	Added	
Retention time, s	10	120	10	120	10	120	10	120	
Basis weight (<i>W</i>), g/m ²	63.8	62.4	73.6	76.6	56.4	60.3	68.1	69.1	
\sqrt{W} , (g/m ²) ^{1/2}	7.99	7.90	8.58	8.75	7.51	7.77	8.25	8.31	
Brightness, %	75.5	75.8	74.9	71.6	77.5	77.0	75.8	75.1	
Specific scattering coefficient, m ² /kg	45	44	44	42	32	27	37	36	
Gray level (<i>V</i>)									
Average(<i>V_{ave}</i>)	45.3	45.6	34.2	32.2	70.8	71.7	49.9	51.3	
Standard deviation(<i>V_{std}</i>)	2.1	2.3	1.7	3.0	4.5	6.7	3.1	5.1	0.36
Optical density (<i>OD</i>)									
Average(<i>OD_{ave}</i>)	0.752	0.750	0.875	0.904	0.559	0.554	0.711	0.700	
Standard deviation(<i>OD_{std}</i>)	0.020	0.022	0.022	0.040	0.028	0.041	0.027	0.043	0.64
<i>OD</i> ²									
Average(<i>OD_{ave}</i> ²)	0.567	0.565	0.769	0.822	0.315	0.310	0.508	0.492	
Standard deviation (<i>OD_{std}</i> ²)	0.030	0.033	0.038	0.072	0.031	0.045	0.038	0.061	0.79
Coefficient of variation	5.3	5.9	5.0	9.0	9.9	14.7	7.6	12.4	0.43
<i>OD_{std}</i> / <i>B</i> , 10 ⁻³ m ² /g	0.31	0.35	0.30	0.52	0.49	0.68	40	63	0.50
(<i>OD_{std}</i>)/ \sqrt{W} , 10 ⁻³ (m ² /g) ^{1/2}	2.5	2.8	2.5	4.6	3.7	5.3	3.3	5.2	0.57
(<i>OD_{std}</i> ²)/ <i>B</i> , 10 ⁻³ m ² /g	47	53	52	95	55	75	57	88	0.86
(<i>OD_{std}</i> ²)/ \sqrt{W} , 10 ⁻³ (m ² /g) ^{1/2}	3.7	4.2	4.4	8.3	4.1	5.9	4.7	7.3	0.79
Subjective ranking of formation (the lower, the better)	0.0	3.6	1.4	6.4	2.3	5.5	3.0	5.8	

Formation analysis

Figure 5 is the scanner images of the 4 kinds of handsheets each regarding retention time and cationic polymer addition, made from hardwood and softwood pulp, respectively. **Table 3** lists several physical properties of the samples. The result of Figure 4 suggested that the average of *OD_{ave}*² would be proportional to Basis weight *W*. But, actually they were not in proportion presumably because softwood pulp has the higher light scattering coefficient *s* and the addition of cationic polymer retained

more calcium carbonate, which increased s , as both found in Table 3. The proportionality seems to apply limitedly to the same furnish.

There are many formation “inhomogeneity” indices that have been proposed from various standpoints. Apart from frequency analyses¹⁰⁾ and floc structure analyses¹¹⁾, formation has been generally analyzed in terms of the coefficient of variation CV of local basis weight^{12,13)}. In this study, a variety of formation indices were calculated from the scanner light transmission images. Firstly, OD and OD^2 were calculated every pixel. Secondly, standard deviation std of Gray level V_{std} , OD and OD^2 , and the coefficient of variation CV (a ratio of the average to std) of OD^2 were calculated. Table 3 summarizes the results as well as the subjective rankings. The eight images in Figure 5 were modified to appear distinctively contrasted at the time of press. So, it may be difficult to connect the images to the statistic results.

Figure 6 shows the propriety of the formation indices to relate to the subjective ranking. The formation indices was normalized so that the average of each index would be 3.5. Among the three standard deviations, that is, V_{std} , OD_{std} and OD^2_{std} , OD^2_{std} was found to distinguish the samples with the fewest reversed pairs. This finding implies that human perception is the most sensitive to the amount convertible to basis weight W . To be more exact, this conversion applies limitedly to paper of uniform structure in terms of fiber source, density, filler content and so on. So, the conversion does not apply to those samples. In spite of the actual discordance, human perception has a scale based on OD^2 . However, CV of OD^2 showed a low Kendall's coefficient r . So, it may be difficult to sense the amount of relative variation accurately. The ratio of OD^2_{std} to W , an index where the average of OD^2 was replaced for W in CV of OD^2 , shows high propriety with r of 0.86. This index distinguished well the eight sheets except HN120. The sheet of HN120 was observed to have many flocs with the order of ca. 5 mm. This order of flocs seems to be striking to visual perception, as Shinozaki¹⁴⁾ showed that the variation in the range of 5.7 to 6.2 mm in wavelength had a high correlation with subjective ranking. OD_{std} and,

particularly, V_{std} were far from propriety as a formation index. V_{std} is sometimes used to estimate formation, but it must be

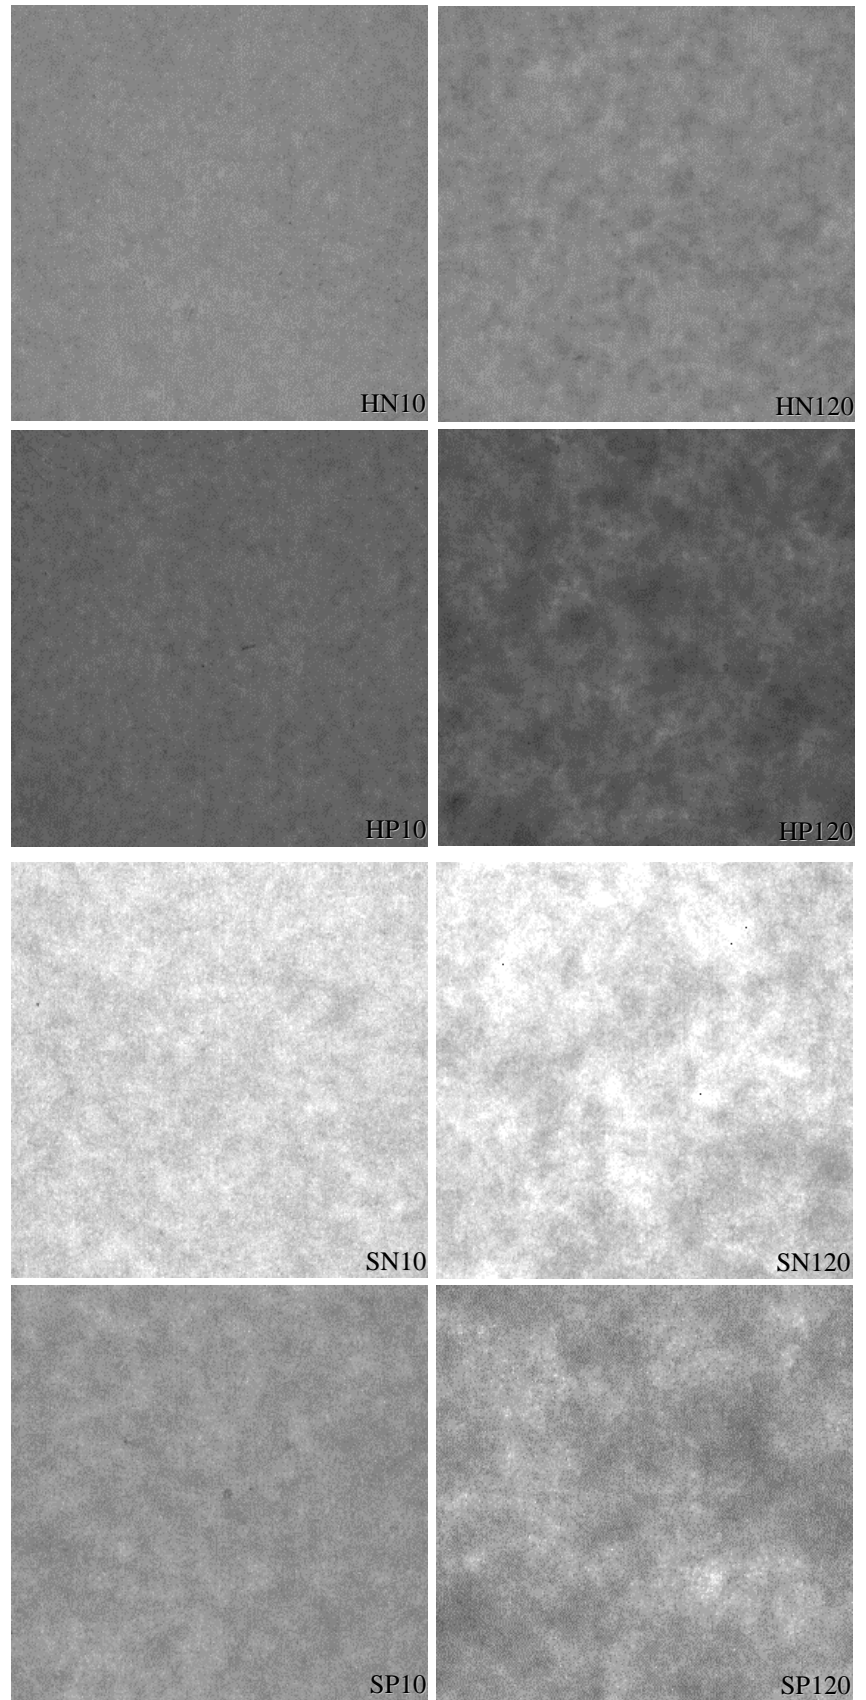


Fig.5 Light transmission images of handsheets made from bleached hardwood kraft pulp. Details are in Table 3.

confined to papers with close gray levels. Kajanto¹⁵⁾ proposed that normalized *Std* (*Std* divided by a root of average both on

REFERENCES

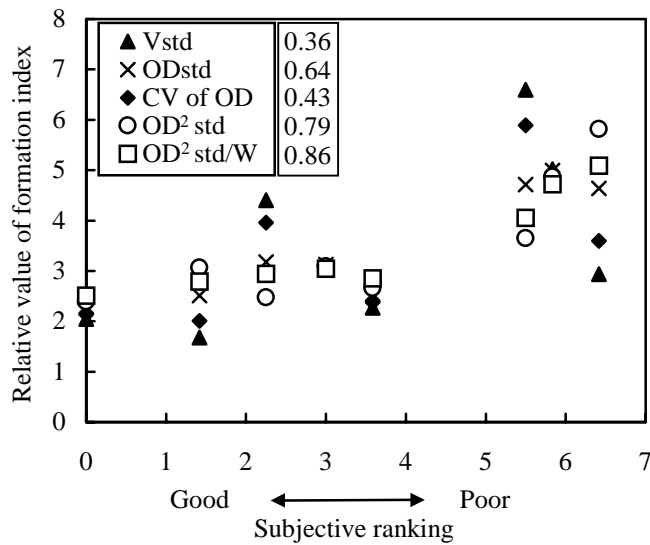


Fig.6 Formation indices and their Kendall's coefficient of correlation. OD^2 -based indices shows better correlation.

the basis of grammage by β -radiography) fitted the appearance better than the coefficient of variation. The normalized *std*, $(OD^2_{ave})/\sqrt{W}$ correlated well but did not function better than $(OD^2_{ave})/W$ in this work, as the other possible indices did not.

CONCLUSIONS

The desk-top flat-bed image scanner with a transparency unit was found to function properly as an image input device for formation analysis under satisfied prerequisite conditions if the output is calibrated based on a standard film or by comparison to Elrepho type reflectometer. However, there remained some distortion in the output characteristics even after the calibration. So, unlike Elrepho type, optical density squared was almost proportional to the basis weight of paper. The formation index, the standard deviation of optical density squared correlated better with the subjective ranking than that of optical density or of gray level. Optical density squared divided by the basis weight showed the highest Kendall's coefficient of correlation. Anyway, the standard deviation of gray level was far from propriety as a formation index.

ACKNOWLEDGMENT

The authors wish to thank the junior students of Biomaterial Sci. Dept. of The Univ. of Tokyo for preparing the handsheets for the formation analysis. The graduate students on Paper science laboratory of The Univ. of Tokyo are thanked for their contribution to the subjective test.

- 1) Davis M N, Roehr W W and Malmstroem H E (1935) An instrument for formation measurement. Paper Trade J 101(July 25): 35-40.
- 2) Anonymous author (1956) Fast-operating formation tester. Paper Trade J 140(April 16): 61.
- 3) Jamison W (1956) New approach to paper formation measurement. Paper Trade J 140(October 8): 30-35.
- 4) Burkhard G, Wrist P E and Mounce G R (1960) A formation tester which graphically records paper structure. Pulp Paper Mag Can 61(6): T319-334.
- 5) Bergh P and Luner P (1983) The application of image analysis to evaluate small scale basis weight variations in paper. Trans. of 7th Intl. Fundamental Research Symp (Vol 2), Mech Eng Publ, London, pp 707-722.
- 6) Shinozaki M, Tajima Y and Miyamoto S (1996) Paper 'formation' image analysis (in Japanese). Japanese J of Paper Technology (Kamipa Gitai) 36(4): 24-28
- 7) Yuhara T, Nakayama S, Arie Y, Kodaka I and Okushima S (1989) Equation of light transmittance of paper for parallel incidence. Proceedings of Japan Tappi pulp and paper research conference 14-17.
- 8) Kubelka P (1947) New contribution to the potics of intensely light-scattering materials. Part I. J Optical Soc of America 38(5): 448-457.
- 9) Hamada H, Enomae T, Onabe F and Saito Y (1999) Colloidal properties of hollow latices and their roles in controlling colorimetric parameters of coated paper surface. Pre-symposium of the 10th ISWPC in press.
- 10) Cresson T and Luner P (1990) The characterization of paper formation analysis. Tappi 73(12): 175-185.
- 11) Dodson C T J and Schaffnit C (1990) Flocculation and orientation effects on paper-formation statistics. Tappi 75(1): 167-171.
- 12) Norman B and Wahren D (1976) Mass distribution and sheet properties of paper. Trans. of 5th Intl. Fundamental Research Symp (Vol 1), Tech Sec, Brit Paper Board Ind Fed, London, pp 7-70.
- 13) Norman B and Wahren D (1972) A comprehensive method for the description of mass distribution in sheets and flocculation and turbulence in suspensions. Svensk Papperstidn 75(11): 807-818.
- 14) Shinozaki M, Tajima Y and Miyamoto S (1998) Formation analysis through multiple regression of light transmission distribution and Fourier transformation analysis (in Japanese). Sen'i Gakkai Preprints 1998(G), Soc Fiber Sci Tech, Japan: G-107

- 15) Kajanto I M, Komppa A and Ritala R K (1989) How formation should be measured and characterized. Nordic Pulp and Paper Res J 4(3): 219-228.